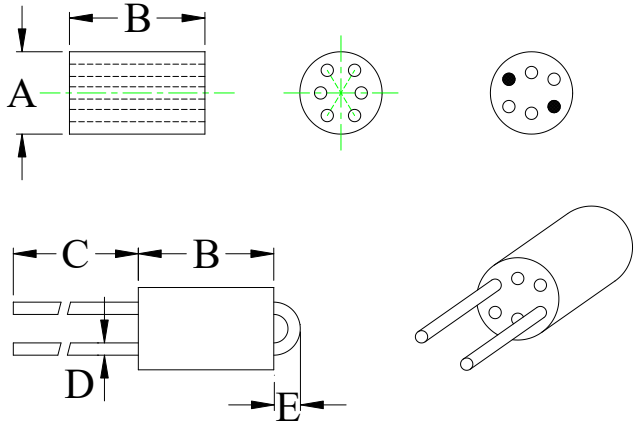


SPECIFICATION FOR APPROVAL

COMMODITY	WIDE BAND CHOKE	SPEC NO.	SP-060927076
ITEM	K5B R6H 1.0Ts Green	版本：A	表單編號：QR-012-02

(1) DIMENSION: (UNIT: mm)		DIM.	TOL.
	A	6.00	± 0.25
	B	10.00	± 0.30
	C	25.00	± 2.00
	D	0.50	± 0.1
	E	1.50	Max

(2) ELECTRICAL CHARACTERISTIC		TEST INSTRUMENTS.
IMPEDANCE at Z 1	58 (min) Ω	☒ AGILENT 4294A Precision Impedance Analyzer ☐ Agilent 4287A RF LCR Meter ☐ AGILENT 4285A Precision L.C.R. ☐ HP-4286A RF L.C.R. Meter. ☐ CHROMA 3302 Automatic Components Analyzer. ☐ WAYNE KERR 6420 Precision Impedance Analyzer. ☐ ZENTECH 1320 BIAS CURRENT. ☐ BK PRECISION 2840 DC Resistance Meter ☐ ZENTECH 502AC Resistance Merter ☐ ADEX AX-1155B DC Low Ohm Meter ☐ WAYNE KERR HI-POT TESTER 7600
IMPEDANCE at Z 2	148 (min) Ω	
IMPEDANCE at Z 3	178 (min) Ω	
TEST FREQUENCY at Z 1	10 MHz	
TEST FREQUENCY at Z 2	50 MHz	
TEST FREQUENCY at Z 3	100 MHz	


REMARK :

PURCHASER CONFIRMED :	APPROVED	CHECKED	DRAWN
			

TEST REPORT

SPEC NO : SP-060927076

Typical Impedance v.s. Frequency Curve

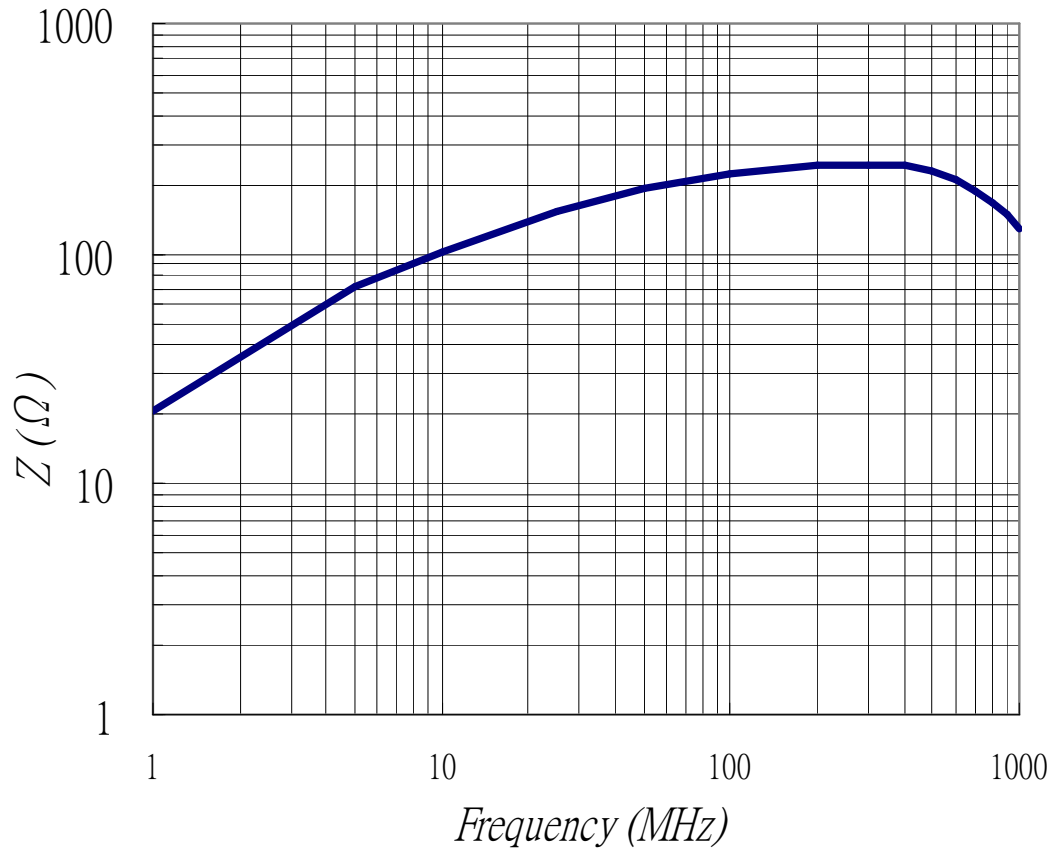

Test Instrument :

HP-4286A RF L.C.R. Meter.

Testing Condition :

Temperature : 25 to 28°C

Humidity : 60 to 70 % RH

Check by :

姜秀琴

Test by :

陳秀月